

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0066
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01908 Calib. Date: 12/08/2014 Calib. No.: 00025
Certification File No.: 01909 Cert. Date: 12/08/2014 Cert. No.: 00022
Linearity File No.: 01910 Lin. Date: 12/08/2014 Lin. No.: 00022
Solution File No.: 01924 Soln. Date: 01/05/2015 Soln. No.: 00186
Sequential File No.: 01924 File Date: 01/05/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0340
Control Solution %: 0.100% Expires: 06/20/2016
Solution Control Lot: 14F130 Bottle No.: 1322

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	20:30S		
Control 1 EC	0.100%	20:31S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:32S		
Control 2 EC	0.099%	20:32S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	20:32S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:33S		
Control 3 EC	0.099%	20:34S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	20:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:35S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: Sgt M Henkel 149

Badge No.: 149

Date: 01/05/2015

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0066
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01908 Calib. Date: 12/08/2014 Calib. No.: 00025
Certification File No.: 01909 Cert. Date: 12/08/2014 Cert. No.: 00022
Linearity File No.: 01910 Lin. Date: 12/08/2014 Lin. No.: 00022
Solution File No.: 01934 Soln. Date: 02/07/2015 Soln. No.: 00187
Sequential File No.: 01934 File Date: 02/07/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0340
Control Solution %: 0.100% Expires: 06/20/2016
Solution Control Lot: 14F130 Bottle No.: 1323

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	00:33S		
Control 1 EC	0.101%	00:33S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	00:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:34S		
Control 2 EC	0.100%	00:35S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	00:35S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:36S		
Control 3 EC	0.099%	00:36S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	00:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:37S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

Sgt M Henkel 149

Badge No.: 149

Date: 02/07/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01908	Calib. Date: 12/08/2014
Certification File No.:	01909	Calib. No.: 00025
Linearity File No.:	01910	Cert. Date: 12/08/2014
Solution File No.:	01942	Cert. No.: 00022
Sequential File No.:	01942	Lin. Date: 12/08/2014
		Lin. No.: 00022
		Soln. Date: 02/22/2015
		Soln. No.: 00188
		File Date: 02/22/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0340
Solution Control Lot:	14F130	Expires: 06/20/2016
		Bottle No.: 1305

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	06:04S		
Control 1 EC	0.102%	06:05S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	06:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:06S		
Control 2 EC	0.100%	06:06S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	06:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:07S		
Control 3 EC	0.099%	06:08S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	06:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:09S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HARTNETT

First Name: JAMES

MI: J

Signature: _____

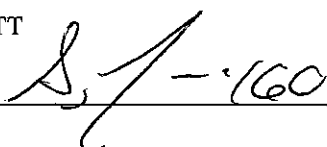

Badge No.: 160

Date: 02/22/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	01908	Calib. Date:	12/08/2014
Certification File No.:	01909	Cert. Date:	12/08/2014
Linearity File No.:	01910	Lin. Date:	12/08/2014
Solution File No.:	01960	Soln. Date:	03/14/2015
Sequential File No.:	01960	File Date:	03/14/2015
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0340
Solution Control Lot:	14F130	Expires:	06/20/2016
		Bottle No.:	1315

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	05:30S		
Control 1 EC	0.103%	05:31S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	05:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:32S		
Control 2 EC	0.100%	05:33S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	05:33S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:33S		
Control 3 EC	0.100%	05:34S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	05:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:35S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HARTNETT

First Name: JAMES

MI: J

Signature: _____



Badge No.: 160

Date: 03/14/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	01908	Calib. Date:	12/08/2014
Certification File No.:	01909	Cert. No.:	00025
Linearity File No.:	01910	Cert. Date:	12/08/2014
Solution File No.:	01976	Lin. No.:	00022
Sequential File No.:	01976	Lin. Date:	12/08/2014
		Soln. Date:	04/05/2015
		Soln. No.:	00190
		File Date:	04/05/2015
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0340
Solution Control Lot:	14F130	Expires:	06/20/2016
		Bottle No.:	1309

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	, or Error(s)
Ambient Air Blank	0.000%	03:51D		
Control 1 EC	0.101%	03:52D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	03:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:53D		
Control 2 EC	0.100%	03:53D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	03:53D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:54D		
Control 3 EC	0.098%	03:55D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	03:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:56D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HARTNETT

First Name: JAMES

MI: J

Signature: _____

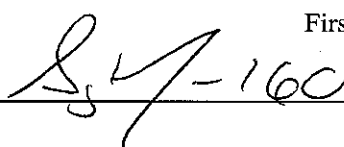

Badge No.: 160

Date: 04/05/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	01908	Calib. Date:	12/08/2014
Certification File No.:	01909	Cert. Date:	12/08/2014
Linearity File No.:	01910	Lin. Date:	12/08/2014
Solution File No.:	01984	Soln. Date:	04/14/2015
Sequential File No.:	01984	File Date:	04/14/2015
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0340
Solution Control Lot:	14F130	Expires:	06/20/2016
		Bottle No.:	1303

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:35D		
Control 1 EC	0.100%	23:36D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	23:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:37D		
Control 2 EC	0.098%	23:37D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	23:37D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:38D		
Control 3 EC	0.098%	23:39D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	23:39D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:40D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL	First Name: GERALD	MI: F.
Signature: <u>Sgt M Henkel 149</u>	Badge No.: 149	Date: 04/14/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	01908	Calib. Date:	12/08/2014
Certification File No.:	01909	Cert. Date:	12/08/2014
Linearity File No.:	01910	Lin. Date:	12/08/2014
Solution File No.:	01993	Soln. Date:	05/12/2015
Sequential File No.:	01993	File Date:	05/12/2015
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0340
Solution Control Lot:	14F130	Expires:	06/20/2016
		Bottle No.:	1317

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	11:58D		
Control 1 EC	0.099%	11:58D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:59D		
Control 2 EC	0.098%	12:00D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	12:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:01D		
Control 3 EC	0.098%	12:01D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	12:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:02D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____

Badge No.: 187

Date: 05/12/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02003	Calib. Date: 09/09/2015
Certification File No.:	02004	Calib. No.: 00026
Linearity File No.:	02005	Cert. Date: 09/09/2015
Solution File No.:	02018	Cert. No.: 00023
Sequential File No.:	02018	Lin. Date: 09/09/2015
		Lin. No.: 00023
		Soln. Date: 11/14/2015
		Soln. No.: 00195
		File Date: 11/14/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	14L135	Expires: 12/31/2016
		Bottle No.: 0052

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:23S		
Control 1 EC	0.101%	08:24S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	08:24S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:25S		
Control 2 EC	0.100%	08:25S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	08:25S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:26S		
Control 3 EC	0.100%	08:27S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	08:27S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:28S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____



Badge No.: 187

Date: 11/14/2015

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0066
Location: PENNSAUKEN TWSP, P.D.
Calibration File No.: 02003 Calib. Date: 09/09/2015 Calib. No.: 00026
Certification File No.: 02004 Cert. Date: 09/09/2015 Cert. No.: 00023
Linearity File No.: 02005 Lin. Date: 09/09/2015 Lin. No.: 00023
Solution File No.: 02011 Soln. Date: 10/10/2015 Soln. No.: 00194
Sequential File No.: 02011 File Date: 10/10/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0341
Control Solution %: 0.100% Expires: 12/31/2016
Solution Control Lot: 14L135 Bottle No.: 0061

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	06:21D		
Control 1 EC	0.100%	06:22D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	06:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:22D		
Control 2 EC	0.100%	06:23D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	06:23D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:24D		
Control 3 EC	0.100%	06:25D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	06:25D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:25D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HARTNETT

First Name: JAMES

MI: J

Signature: _____

Badge No.: 160

Date: 10/10/2015

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0066
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02003	Calib. Date: 09/09/2015
Certification File No.:	02004	Calib. No.: 00026
Linearity File No.:	02005	Cert. Date: 09/09/2015
Solution File No.:	02028	Cert. No.: 00023
Sequential File No.:	02028	Lin. Date: 09/09/2015
		Lin. No.: 00023
		Soln. Date: 12/17/2015
		Soln. No.: 00196
		File Date: 12/17/2015
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0341
Solution Control Lot:	14L135	Expires: 12/31/2016
		Bottle No.: 0066

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:49S		
Control 1 EC	0.101%	09:50S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	09:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:51S		
Control 2 EC	0.100%	09:51S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	09:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:52S		
Control 3 EC	0.101%	09:53S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:53S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:54S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____



#187

Badge No.: 187

Date: 12/17/2015