

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARUM-0051 |
| Location: | PENNSAUKEN TWSP. P.D. | |
| Calibration File No.: | 01711 | Calib. Date: 07/28/2011 |
| Certification File No.: | 01712 | Calib. No.: 00017 |
| Linearity File No.: | 01713 | Cert. Date: 07/28/2011 |
| Solution File No.: | 01772 | Cert. No.: 00013 |
| Sequential File No.: | 01772 | Lin. Date: 07/28/2011 |
| | | Lin. No.: 00013 |
| | | Soln. Date: 12/13/2011 |
| | | Soln. No.: 00160 |
| | | File Date: 12/13/2011 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDUN S3-0340 |
| Solution Control Lot: | 11C088 | Expires: 03/31/2013 |
| | | Bottle No.: 0179 |

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 21:28S | | |
| Control 1 EC | 0.100% | 21:28S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.101% | 21:28S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 21:29S | | |
| Control 2 EC | 0.099% | 21:29S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.099% | 21:29S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 21:30S | | |
| Control 3 EC | 0.100% | 21:31S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 21:31S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 21:31S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

PK M Henkel 149

Badge No.: 149

Date: 12/13/2011

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARUM-0051 |
| Location: | PENNSAUKEN TWSP. P.D. | |
| Calibration File No.: | 01711 | Calib. Date: 07/28/2011 |
| Certification File No.: | 01712 | Cert. No.: 00017 |
| Linearity File No.: | 01713 | Cert. Date: 07/28/2011 |
| Solution File No.: | 01762 | Lin. No.: 00013 |
| Sequential File No.: | 01762 | Lin. Date: 07/28/2011 |
| | | Soln. No.: 00159 |
| | | Soln. Date: 11/20/2011 |
| | | File Date: 11/20/2011 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDUN S3-0340 |
| Solution Control Lot: | 11C088 | Expires: 03/31/2013 |
| | | Bottle No.: 0180 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 02:43S | | |
| Control 1 EC | 0.100% | 02:43S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.099% | 02:43S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 02:44S | | |
| Control 2 EC | 0.099% | 02:45S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 02:45S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 02:45S | | |
| Control 3 EC | 0.100% | 02:46S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.099% | 02:46S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 02:47S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

PH HENKEL 149

Badge No.: 149

Date: 11/20/2011

Calibrating Unit

New Standard Solution Report

| | | | |
|-------------------------|-----------------------|--------------|--------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: | ARUM-0051 |
| Location: | PENNSAUKEN TWSP. P.D. | | |
| Calibration File No.: | 01711 | Calib. Date: | 07/28/2011 |
| Certification File No.: | 01712 | Cert. No.: | 00017 |
| Linearity File No.: | 01713 | Cert. Date: | 07/28/2011 |
| Solution File No.: | 01747 | Lin. No.: | 00013 |
| Sequential File No.: | 01747 | Lin. Date: | 07/28/2011 |
| | | Soln. Date: | 10/20/2011 |
| | | Soln. No.: | 00158 |
| | | File Date: | 10/20/2011 |
| | | | |
| Calibrating Unit: | WET | Model No.: | CU-34 |
| Control Solution %: | 0.100% | Serial No.: | DDUN S3-0340 |
| Solution Control Lot: | 10J083 | Expires: | 10/04/2012 |
| | | Bottle No.: | 1179 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 13:04D | | |
| Control 1 EC | 0.099% | 13:05D | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.099% | 13:05D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:05D | | |
| Control 2 EC | 0.099% | 13:06D | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 13:06D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:07D | | |
| Control 3 EC | 0.099% | 13:07D | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.099% | 13:07D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:08D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature:

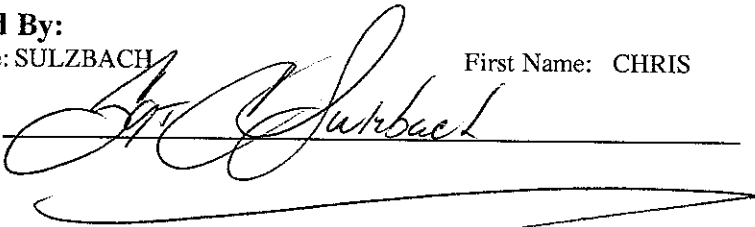

Badge No.: 127

Date: 10/20/2011

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARUM-0051 |
| Location: | PENNSAUKEN TWSP. P.D. | |
| Calibration File No.: | 01711 | Calib. Date: 07/28/2011 |
| Certification File No.: | 01712 | Calib. No.: 00017 |
| Linearity File No.: | 01713 | Cert. Date: 07/28/2011 |
| Solution File No.: | 01740 | Lin. No.: 00013 |
| Sequential File No.: | 01740 | Soln. Date: 09/22/2011 |
| | | Soln. No.: 00157 |
| | | File Date: 09/22/2011 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDUN S3-0340 |
| Solution Control Lot: | 10J083 | Expires: 10/04/2012 |
| | | Bottle No.: 1184 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 09:04D | | |
| Control 1 EC | 0.098% | 09:05D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.098% | 09:05D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:05D | | |
| Control 2 EC | 0.098% | 09:06D | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.098% | 09:06D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:06D | | |
| Control 3 EC | 0.098% | 09:07D | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.098% | 09:07D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:08D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: _____



Badge No.: 127

Date: 09/22/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01711 Calib. Date: 07/28/2011 Calib. No.: 00017
Certification File No.: 01712 Cert. Date: 07/28/2011 Cert. No.: 00013
Linearity File No.: 01713 Lin. Date: 07/28/2011 Lin. No.: 00013
Solution File No.: 01732 Soln. Date: 08/25/2011 Soln. No.: 00156
Sequential File No.: 01732 File Date: 08/25/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0340
Control Solution %: 0.100% Expires: 10/04/2012
Solution Control Lot: 10J083 Bottle No.: 1178

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 11:48D | | |
| Control 1 EC | 0.098% | 11:48D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.098% | 11:48D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:49D | | |
| Control 2 EC | 0.098% | 11:49D | 33.9°C | *** TEST PASSED *** |
| Control 2 IR | 0.099% | 11:49D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:50D | | |
| Control 3 EC | 0.098% | 11:51D | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.097% | 11:51D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 11:51D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: _____



Badge No.: 127

Date: 08/25/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01711 Calib. Date: 07/28/2011 Calib. No.: 00017
Certification File No.: 01712 Cert. Date: 07/28/2011 Cert. No.: 00013
Linearity File No.: 01713 Lin. Date: 07/28/2011 Lin. No.: 00013
Solution File No.: 01722 Soln. Date: 08/08/2011 Soln. No.: 00155
Sequential File No.: 01722 File Date: 08/08/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0340
Control Solution %: 0.100% Expires: 10/04/2012
Solution Control Lot: 10J083 Bottle No.: 1177

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 16:11D | | |
| Control 1 EC | 0.098% | 16:12D | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.098% | 16:12D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 16:12D | | |
| Control 2 EC | 0.098% | 16:13D | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.096% | 16:13D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 16:14D | | |
| Control 3 EC | 0.097% | 16:14D | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.097% | 16:14D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 16:15D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: _____



Badge No.: 127

Date: 08/08/2011

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARUM-0051 |
| Location: | PENNSAUKEN TWSP. P.D. | |
| Calibration File No.: | 01696 | Calib. Date: 06/16/2011 |
| Certification File No.: | 01697 | Calib. No.: 00016 |
| Linearity File No.: | 01698 | Cert. Date: 06/16/2011 |
| Solution File No.: | 01703 | Lin. No.: 00012 |
| Sequential File No.: | 01703 | Soln. Date: 07/02/2011 |
| | | Soln. No.: 00153 |
| | | File Date: 07/02/2011 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDUN S3-0340 |
| Solution Control Lot: | 10J083 | Expires: 10/04/2012 |
| | | Bottle No.: 1190 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 07:07D | | |
| Control 1 EC | 0.097% | 07:08D | 33.9°C | *** TEST PASSED *** |
| Control 1 IR | 0.097% | 07:08D | 33.9°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 07:08D | | |
| Control 2 EC | 0.097% | 07:09D | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.096% | 07:09D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 07:09D | | |
| Control 3 EC | 0.096% | 07:10D | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.097% | 07:10D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 07:11D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SANDERS

First Name: JAMES

MI: R

Signature: _____

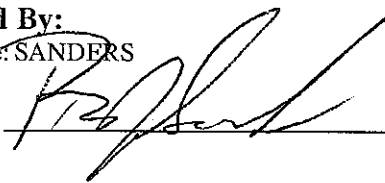

Badge No.: 126

Date: 07/02/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01651 Calib. Date: 03/16/2011 Calib. No.: 00015
Certification File No.: 01652 Cert. Date: 03/16/2011 Cert. No.: 00011
Linearity File No.: 01653 Lin. Date: 03/16/2011 Lin. No.: 00011
Solution File No.: 01694 Soln. Date: 06/13/2011 Soln. No.: 00151
Sequential File No.: 01694 File Date: 06/13/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0341
Control Solution %: 0.100% Expires: 10/04/2012
Solution Control Lot: 10J083 Bottle No.: 1197

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 15:07D | | |
| Control 1 EC | 0.098% | 15:07D | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.099% | 15:07D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 15:08D | | |
| Control 2 EC | 0.099% | 15:08D | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.099% | 15:08D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 15:09D | | |
| Control 3 EC | 0.099% | 15:09D | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.098% | 15:09D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 15:10D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: _____



Badge No.: 127

Date: 06/13/2011

Calibrating Unit

New Standard Solution Report

| | | | |
|-------------------------|-----------------------|--------------|--------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: | ARUM-0051 |
| Location: | PENNSAUKEN TWSP. P.D. | | |
| Calibration File No.: | 01651 | Calib. Date: | 03/16/2011 |
| Certification File No.: | 01652 | Cert. No.: | 00015 |
| Linearity File No.: | 01653 | Cert. Date: | 03/16/2011 |
| Solution File No.: | 01680 | Lin. No.: | 00011 |
| Sequential File No.: | 01680 | Soln. Date: | 05/17/2011 |
| | | Soln. No.: | 00150 |
| | | File Date: | 05/17/2011 |
| | | | |
| Calibrating Unit: | WET | Model No.: | CU-34 |
| Control Solution %: | 0.100% | Serial No.: | DDUN S3-0341 |
| Solution Control Lot: | 10J083 | Expires: | 10/04/2012 |
| | | Bottle No.: | 1195 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 23:52D | | |
| Control 1 EC | 0.099% | 23:52D | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.099% | 23:52D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 23:53D | | |
| Control 2 EC | 0.099% | 23:53D | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.100% | 23:53D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 23:54D | | |
| Control 3 EC | 0.099% | 23:55D | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.098% | 23:55D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 23:55D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

Handwritten Signature 149

Badge No.: 149

Date: 05/17/2011

Calibrating Unit New Standard Solution Report

| | | | |
|-------------------------|-----------------------|--------------|--------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: | ARUM-0051 |
| Location: | PENNSAUKEN TWSP. P.D. | | |
| Calibration File No.: | 01651 | Calib. Date: | 03/16/2011 |
| Certification File No.: | 01652 | Cert. No.: | 00015 |
| Linearity File No.: | 01653 | Cert. Date: | 03/16/2011 |
| Solution File No.: | 01669 | Lin. Date: | 03/16/2011 |
| Sequential File No.: | 01669 | Soln. Date: | 04/16/2011 |
| | | File Date: | 04/16/2011 |
| Calibrating Unit: | WET | Model No.: | CU-34 |
| Control Solution %: | 0.100% | Serial No.: | DDUN S3-0341 |
| Solution Control Lot: | 10J083 | Expires: | 10/04/2012 |
| | | Bottle No.: | 1194 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 16:37D | | |
| Control 1 EC | 0.100% | 16:37D | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.099% | 16:37D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 16:38D | | |
| Control 2 EC | 0.100% | 16:39D | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.101% | 16:39D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 16:39D | | |
| Control 3 EC | 0.101% | 16:40D | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 16:40D | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 16:40D | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: HERTLINE III

First Name: WILLIAM

MI: C

Signature: _____



Badge No.: 159

Date: 04/16/2011

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01557 Calib. Date: 12/22/2010 Calib. No.: 00012
Certification File No.: 01558 Cert. Date: 12/22/2010 Cert. No.: 00010
Linearity File No.: 01559 Lin. Date: 12/22/2010 Lin. No.: 00010
Solution File No.: 01635 Soln. Date: 02/25/2011 Soln. No.: 00143
Sequential File No.: 01635 File Date: 02/25/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0341
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 0571

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 13:48S | | |
| Control 1 EC | 0.100% | 13:49S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 13:49S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:50S | | |
| Control 2 EC | 0.098% | 13:50S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.101% | 13:50S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:51S | | |
| Control 3 EC | 0.099% | 13:52S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 13:52S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:53S | | |

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

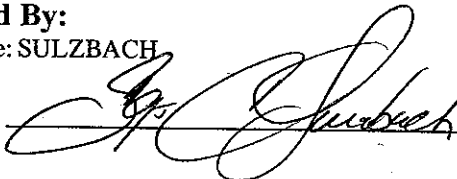Signature: 

Badge No.: 127

Date: 02/25/2011

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: PENNSAUKEN TWSP. P.D. Serial No.: ARUM-0051
Calibration File No.: 01557 Calib. Date: 12/22/2010 Calib. No.: 00012
Certification File No.: 01558 Cert. Date: 12/22/2010 Cert. No.: 00010
Linearity File No.: 01559 Lin. Date: 12/22/2010 Lin. No.: 00010
Solution File No.: 01633 Soln. Date: 02/24/2011 Soln. No.: 00142
Sequential File No.: 01633 File Date: 02/24/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0341
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 0551

| Function | Result | Time | Temperature | Comment(s) or Error(s) |
|-------------------|--------|--------|----------------|------------------------|
| | %BAC | HH:MM | Simulator (°C) | |
| Ambient Air Blank | 0.000% | 03:34S | | |
| Control 1 EC | 0.100% | 03:34S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.100% | 03:34S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 03:35S | | |
| Control 2 EC | 0.098% | 03:36S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.101% | 03:36S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 03:37S | | |
| Control 3 EC | 0.097% | 03:37S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 03:37S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 03:38S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MOLES

First Name: VITO

MI: M

Signature: _____

Badge No.: 171

Date: 02/24/2011

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARUM-0051 |
| Location: | PENNSAUKEN TWSP. P.D. | |
| Calibration File No.: | 01557 | Calib. Date: 12/22/2010 |
| Certification File No.: | 01558 | Calib. No.: 00012 |
| Linearity File No.: | 01559 | Cert. Date: 12/22/2010 |
| Solution File No.: | 01621 | Cert. No.: 00010 |
| Sequential File No.: | 01621 | Lin. Date: 12/22/2010 |
| | | Lin. No.: 00010 |
| | | Soln. Date: 02/19/2011 |
| | | Soln. No.: 00141 |
| | | File Date: 02/19/2011 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDUN S3-0341 |
| Solution Control Lot: | 10C077 | Expires: 03/10/2012 |
| | | Bottle No.: 0567 |

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 21:45S | | |
| Control 1 EC | 0.100% | 21:45S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.103% | 21:45S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 21:46S | | |
| Control 2 EC | 0.099% | 21:47S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.101% | 21:47S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 21:48S | | |
| Control 3 EC | 0.100% | 21:48S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.101% | 21:48S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 21:49S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KERN

First Name: RAYMOND

MI: T

Signature: _____

Ray Kern #181

Badge No.: 181

Date: 02/19/2011

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARUM-0051 |
| Location: | PENNSAUKEN TWSP. P.D. | |
| Calibration File No.: | 01557 | Calib. Date: 12/22/2010 |
| Certification File No.: | 01558 | Calib. No.: 00012 |
| Linearity File No.: | 01559 | Cert. Date: 12/22/2010 |
| Solution File No.: | 01614 | Cert. No.: 00010 |
| Sequential File No.: | 01614 | Lin. Date: 12/22/2010 |
| | | Lin. No.: 00010 |
| | | Soln. Date: 02/16/2011 |
| | | Soln. No.: 00140 |
| | | File Date: 02/16/2011 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDUN S3-0341 |
| Solution Control Lot: | 10C077 | Expires: 03/10/2012 |
| | | Bottle No.: 0562 |

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 00:05S | | |
| Control 1 EC | 0.101% | 00:05S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.103% | 00:05S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 00:06S | | |
| Control 2 EC | 0.099% | 00:07S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.099% | 00:07S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 00:08S | | |
| Control 3 EC | 0.099% | 00:08S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.099% | 00:08S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 00:09S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KERN

First Name: RAYMOND

MI: T

Signature: _____

Ray Kern #181

Badge No.: 181

Date: 02/16/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01557 Calib. Date: 12/22/2010 Calib. No.: 00012
Certification File No.: 01558 Cert. Date: 12/22/2010 Cert. No.: 00010
Linearity File No.: 01559 Lin. Date: 12/22/2010 Lin. No.: 00010
Solution File No.: 01605 Soln. Date: 02/06/2011 Soln. No.: 00139
Sequential File No.: 01605 File Date: 02/06/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0341
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 0557

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 09:38S | | |
| Control 1 EC | 0.101% | 09:38S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.101% | 09:38S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:39S | | |
| Control 2 EC | 0.100% | 09:40S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.101% | 09:40S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:41S | | |
| Control 3 EC | 0.099% | 09:41S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.099% | 09:41S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:42S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: _____

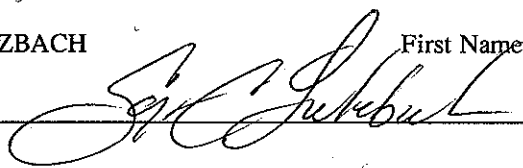

Badge No.: 127

Date: 02/06/2011

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01557 Calib. Date: 12/22/2010 Calib. No.: 00012
Certification File No.: 01558 Cert. Date: 12/22/2010 Cert. No.: 00010
Linearity File No.: 01559 Lin. Date: 12/22/2010 Lin. No.: 00010
Solution File No.: 01593 Soln. Date: 01/26/2011 Soln. No.: 00138
Sequential File No.: 01593 File Date: 01/26/2011

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0341
Control Solution %: 0.100% Expires: 03/10/2012
Solution Control Lot: 10C077 Bottle No.: 0566

| Function | Result | Time | Temperature | Comment(s) |
|-------------------|--------|--------|----------------|---------------------|
| | %BAC | HH:MM | Simulator (°C) | or Error(s) |
| Ambient Air Blank | 0.000% | 10:41S | | |
| Control 1 EC | 0.101% | 10:42S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.101% | 10:42S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:43S | | |
| Control 2 EC | 0.100% | 10:43S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.101% | 10:43S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:44S | | |
| Control 3 EC | 0.100% | 10:45S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 10:45S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 10:46S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: _____



Badge No.: 127

Date: 01/26/2011

Calibrating Unit

New Standard Solution Report

| | | |
|-------------------------|-----------------------|--------------------------|
| Equipment | Alcotest 7110 MKIII-C | Serial No.: ARUM-0051 |
| Location: | PENNSAUKEN TWSP. P.D. | |
| Calibration File No.: | 01557 | Calib. Date: 12/22/2010 |
| Certification File No.: | 01558 | Calib. No.: 00012 |
| Linearity File No.: | 01559 | Cert. Date: 12/22/2010 |
| Solution File No.: | 01584 | Cert. No.: 00010 |
| Sequential File No.: | 01584 | Lin. Date: 12/22/2010 |
| | | Lin. No.: 00010 |
| | | Soln. Date: 01/17/2011 |
| | | Soln. No.: 00136 |
| | | File Date: 01/17/2011 |
| | | |
| Calibrating Unit: | WET | Model No.: CU-34 |
| Control Solution %: | 0.100% | Serial No.: DDUN S3-0341 |
| Solution Control Lot: | 10C077 | Expires: 03/10/2012 |
| | | Bottle No.: 0554 |

| Function | Result %BAC | Time HH:MM | Temperature Simulator (°C) | Comment(s) or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000% | 09:15S | | |
| Control 1 EC | 0.101% | 09:16S | 34.0°C | *** TEST PASSED *** |
| Control 1 IR | 0.102% | 09:16S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:17S | | |
| Control 2 EC | 0.100% | 09:17S | 34.0°C | *** TEST PASSED *** |
| Control 2 IR | 0.101% | 09:17S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:18S | | |
| Control 3 EC | 0.100% | 09:19S | 34.0°C | *** TEST PASSED *** |
| Control 3 IR | 0.100% | 09:19S | 34.0°C | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 09:20S | | |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: _____

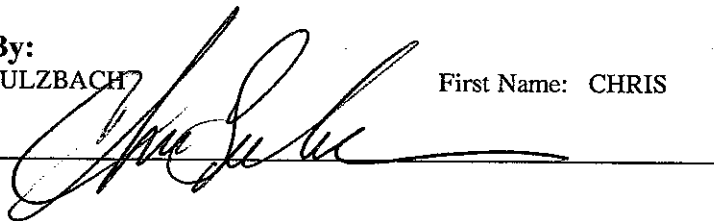

Badge No.: 127

Date: 01/17/2011