

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01911	Calib. Date: 10/16/2012
Certification File No.:	01912	Calib. No.: 00020
Linearity File No.:	01913	Cert. Date: 10/16/2012
Solution File No.:	01949	Cert. No.: 00017
Sequential File No.:	01949	Lin. Date: 10/16/2012
		Lin. No.: 00016
		Soln. Date: 12/15/2012
		Soln. No.: 00177
		File Date: 12/15/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	12C100	Expires: 03/02/2014
		Bottle No.: 1200

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:01S		
Control 1 EC	0.101%	19:02S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	19:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:03S		
Control 2 EC	0.100%	19:03S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	19:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:04S		
Control 3 EC	0.100%	19:05S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	19:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:05S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____

Badge No.: 187

Date: 12/15/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01911	Calib. Date: 10/16/2012
Certification File No.:	01912	Calib. No.: 00020
Linearity File No.:	01913	Cert. Date: 10/16/2012
Solution File No.:	01937	Cert. No.: 00017
Sequential File No.:	01937	Lin. Date: 10/16/2012
		Lin. No.: 00016
		Soln. Date: 11/20/2012
		Soln. No.: 00176
		File Date: 11/20/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	12C100	Expires: 03/02/2014
		Bottle No.: 1191

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:58S		
Control 1 EC	0.101%	16:59S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:00S		
Control 2 EC	0.100%	17:00S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	17:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:01S		
Control 3 EC	0.100%	17:02S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	17:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:02S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KUCHMEK

First Name: JOSEPH

MI: -

Signature:  #190

Badge No.: 190

Date: 11/20/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01911 Calib. Date: 10/16/2012 Calib. No.: 00020
Certification File No.: 01912 Cert. Date: 10/16/2012 Cert. No.: 00017
Linearity File No.: 01913 Lin. Date: 10/16/2012 Lin. No.: 00016
Solution File No.: 01926 Soln. Date: 11/02/2012 Soln. No.: 00175
Sequential File No.: 01926 File Date: 11/02/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0338
Control Solution %: 0.100% Expires: 03/02/2014
Solution Control Lot: 12C100 Bottle No.: 1193

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:16S		
Control 1 EC	0.101%	04:17S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	04:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:18S		
Control 2 EC	0.100%	04:18S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	04:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:19S		
Control 3 EC	0.100%	04:20S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	04:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:20S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KUCHMEK

First Name: JOSEPH

MI: -

Signature:  #190

Badge No.: 190

Date: 11/02/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01826 Calib. Date: 05/01/2012 Calib. No.: 00019
Certification File No.: 01827 Cert. Date: 05/01/2012 Cert. No.: 00016
Linearity File No.: 01828 Lin. Date: 05/01/2012 Lin. No.: 00015
Solution File No.: 01899 Soln. Date: 09/28/2012 Soln. No.: 00173
Sequential File No.: 01899 File Date: 09/28/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0338
Control Solution %: 0.100% Expires: 03/02/2014
Solution Control Lot: 12C100 Bottle No.: 1176

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:53D		
Control 1 EC	0.098%	19:54D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	19:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:54D		
Control 2 EC	0.098%	19:55D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	19:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:56D		
Control 3 EC	0.098%	19:56D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	19:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:57D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

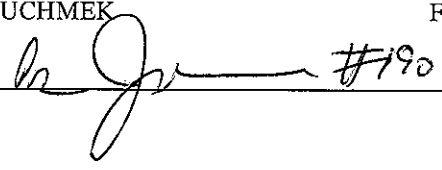
Changed By:

Last Name: KUCHMEK

First Name: JOSEPH

MI: -

Signature: _____



Badge No.: 190

Date: 09/28/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01826 Calib. Date: 05/01/2012 Calib. No.: 00019
Certification File No.: 01827 Cert. Date: 05/01/2012 Cert. No.: 00016
Linearity File No.: 01828 Lin. Date: 05/01/2012 Lin. No.: 00015
Solution File No.: 01886 Soln. Date: 09/13/2012 Soln. No.: 00172
Sequential File No.: 01886 File Date: 09/13/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0338
Control Solution %: 0.100% Expires: 03/02/2014
Solution Control Lot: 12C100 Bottle No.: 1192

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:12D		
Control 1 EC	0.098%	06:13D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	06:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:13D		
Control 2 EC	0.098%	06:14D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	06:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:14D		
Control 3 EC	0.097%	06:15D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	06:15D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:16D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: _____

P.F. 187

Badge No.: 187

Date: 09/13/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01826	Calib. Date: 05/01/2012
Certification File No.:	01827	Calib. No.: 00019
Linearity File No.:	01828	Cert. Date: 05/01/2012
Solution File No.:	01873	Cert. No.: 00016
Sequential File No.:	01873	Lin. Date: 05/01/2012
		Lin. No.: 00015
		Soln. Date: 08/20/2012
		Soln. No.: 00171
		File Date: 08/20/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	12C100	Expires: 03/02/2014
		Bottle No.: 1182

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:18D		
Control 1 EC	0.098%	06:18D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	06:18D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:19D		
Control 2 EC	0.097%	06:20D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.097%	06:20D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:20D		
Control 3 EC	0.097%	06:21D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	06:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:21D		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KUCHMEK

First Name: JOSEPH

MI: -

Signature: 

Badge No.: 190

Date: 08/20/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01826	Calib. Date: 05/01/2012
Certification File No.:	01827	Calib. No.: 00019
Linearity File No.:	01828	Cert. Date: 05/01/2012
Solution File No.:	01864	Cert. No.: 00016
Sequential File No.:	01864	Lin. Date: 05/01/2012
		Lin. No.: 00015
		Soln. Date: 08/04/2012
		Soln. No.: 00170
		File Date: 08/04/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	12C100	Expires: 03/02/2014
		Bottle No.: 1189

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:55D		
Control 1 EC	0.100%	00:55D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	00:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:56D		
Control 2 EC	0.099%	00:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	00:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:57D		
Control 3 EC	0.099%	00:58D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	00:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:58D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: _____

Gerald Henkel 149

Badge No.: 149

Date: 08/04/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01826 Calib. Date: 05/01/2012 Calib. No.: 00019
Certification File No.: 01827 Cert. Date: 05/01/2012 Cert. No.: 00016
Linearity File No.: 01828 Lin. Date: 05/01/2012 Lin. No.: 00015
Solution File No.: 01853 Soln. Date: 07/13/2012 Soln. No.: 00169
Sequential File No.: 01853 File Date: 07/13/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0338
Control Solution %: 0.100% Expires: 03/02/2014
Solution Control Lot: 12C100 Bottle No.: 1178

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:11D		
Control 1 EC	0.099%	01:12D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	01:12D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:13D		
Control 2 EC	0.099%	01:13D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	01:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:14D		
Control 3 EC	0.099%	01:14D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	01:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:15D		

All tests within acceptable tolerance.

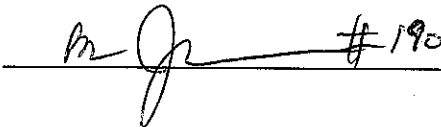
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KUCHMEK

First Name: JOSEPH

MI: -

Signature:  #190

Badge No.: 190

Date: 07/13/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01826	Calib. Date: 05/01/2012
Certification File No.:	01827	Calib. No.: 00019
Linearity File No.:	01828	Cert. Date: 05/01/2012
Solution File No.:	01846	Cert. No.: 00016
Sequential File No.:	01846	Lin. Date: 05/01/2012
		Lin. No.: 00015
		Soln. Date: 06/17/2012
		Soln. No.: 00168
		File Date: 06/17/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	12C100	Expires: 03/02/2014
		Bottle No.: 1180

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	22:04D		
Control 1 EC	0.097%	22:04D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.097%	22:04D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:05D		
Control 2 EC	0.097%	22:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	22:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:06D		
Control 3 EC	0.097%	22:07D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	22:07D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:07D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: PETER

MI: E

Signature: _____

Badge No.: 187

Date: 06/17/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01826	Calib. Date: 05/01/2012
Certification File No.:	01827	Calib. No.: 00019
Linearity File No.:	01828	Cert. Date: 05/01/2012
Solution File No.:	01838	Cert. No.: 00016
Sequential File No.:	01838	Lin. Date: 05/01/2012
		Lin. No.: 00015
		Soln. Date: 05/24/2012
		Soln. No.: 00167
		File Date: 05/24/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	11C088	Expires: 03/31/2013
		Bottle No.: 0196

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:05D		
Control 1 EC	0.100%	04:05D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	04:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:06D		
Control 2 EC	0.100%	04:06D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	04:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:07D		
Control 3 EC	0.099%	04:08D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	04:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: FABIANI

First Name: PETER

MI: E

Signature: _____



Badge No.: 187

Date: 05/24/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	01781	Calib. Date: 01/26/2012
Certification File No.:	01782	Calib. No.: 00018
Linearity File No.:	01783	Cert. Date: 01/26/2012
Solution File No.:	01819	Lin. No.: 00015
Sequential File No.:	01819	Lin. Date: 01/26/2012
		Soln. No.: 00165
		Soln. Date: 04/18/2012
		File Date: 04/18/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0340
Solution Control Lot:	11C088	Expires: 03/31/2013
		Bottle No.: 0198

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	04:12D		
Control 1 EC	0.099%	04:12D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:12D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:13D		
Control 2 EC	0.098%	04:13D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	04:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:14D		
Control 3 EC	0.099%	04:15D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	04:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:16D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: FABIANI

First Name: PETER

MI: E

Signature: _____

[Handwritten Signature] #187

Badge No.: 187

Date: 04/18/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01781 Calib. Date: 01/26/2012 Calib. No.: 00018
Certification File No.: 01782 Cert. Date: 01/26/2012 Cert. No.: 00015
Linearity File No.: 01783 Lin. Date: 01/26/2012 Lin. No.: 00014
Solution File No.: 01805 Soln. Date: 03/21/2012 Soln. No.: 00164
Sequential File No.: 01805 File Date: 03/21/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0340
Control Solution %: 0.100% Expires: 03/31/2013
Solution Control Lot: 11C088 Bottle No.: 0195

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:10S		
Control 1 EC	0.098%	16:11S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	16:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:11S		
Control 2 EC	0.098%	16:12S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:13S		
Control 3 EC	0.099%	16:13S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	16:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:14S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: KUCHMEK

First Name: JOSEPH

MI: -

Signature: _____

 #180

Badge No.: 190

Date: 03/21/2012

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.
Calibration File No.: 01781 Calib. Date: 01/26/2012 Calib. No.: 00018
Certification File No.: 01782 Cert. Date: 01/26/2012 Cert. No.: 00015
Linearity File No.: 01783 Lin. Date: 01/26/2012 Lin. No.: 00014
Solution File No.: 01794 Soln. Date: 02/27/2012 Soln. No.: 00163
Sequential File No.: 01794 File Date: 02/27/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0340
Control Solution %: 0.100% Expires: 03/31/2013
Solution Control Lot: 11C088 Bottle No.: 0192

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:13S		
Control 1 EC	0.100%	08:13S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	08:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:14S		
Control 2 EC	0.099%	08:15S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	08:15S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:16S		
Control 3 EC	0.099%	08:16S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	08:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:17S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: SAMPSON

First Name: SHAUN

MI: .

Signature:  # 142

Badge No.: 142

Date: 02/27/2012

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	01711	Calib. Date:	07/28/2011
Certification File No.:	01712	Cert. No.:	00017
Linearity File No.:	01713	Cert. Date:	07/28/2011
Solution File No.:	01779	Lin. No.:	00013
Sequential File No.:	01779	Soln. Date:	01/19/2012
		Soln. No.:	00161
		File Date:	01/19/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0340
Solution Control Lot:	11C088	Expires:	03/31/2013
		Bottle No.:	0194

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:02S		
Control 1 EC	0.100%	04:03S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	04:03S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:04S		
Control 2 EC	0.099%	04:04S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	04:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:05S		
Control 3 EC	0.099%	04:06S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	04:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:06S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: *File M Henkel 149*

Badge No.: 149

Date: 01/19/2012