

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02382	Calib. Date: 11/25/2015
Certification File No.:	02383	Calib. No.: 00029
Linearity File No.:	02384	Cert. Date: 11/25/2015
Solution File No.:	02400	Cert. No.: 00025
Sequential File No.:	02400	Lin. Date: 11/25/2015
		Lin. No.: 00024
		Soln. Date: 01/17/2016
		Soln. No.: 00240
		File Date: 01/17/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	14L135	Expires: 12/31/2016
		Bottle No.: 0065

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:39S		
Control 1 EC	0.100%	09:40S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:40S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:40S		
Control 2 EC	0.098%	09:41S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:42S		
Control 3 EC	0.098%	09:42S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	09:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:43S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: REESE

First Name: STEVEN

MI: R

Signature: \_\_\_\_\_

*Mr. S. Reese #137*

Badge No.: 137

Date: 01/17/2016

# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARUM-0051  
Location: PENNSAUKEN TWSP. P.D.  
Calibration File No.: 02382 Calib. Date: 11/25/2015 Calib. No.: 00029  
Certification File No.: 02383 Cert. Date: 11/25/2015 Cert. No.: 00025  
Linearity File No.: 02384 Lin. Date: 11/25/2015 Lin. No.: 00024  
Solution File No.: 02407 Soln. Date: 02/11/2016 Soln. No.: 00241  
Sequential File No.: 02407 File Date: 02/11/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0338  
Control Solution %: 0.100% Expires: 12/31/2016  
Solution Control Lot: 14L135 Bottle No.: 0068

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:48S		
Control 1 EC	0.099%	03:49S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	03:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:50S		
Control 2 EC	0.097%	03:50S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	03:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:51S		
Control 3 EC	0.097%	03:52S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	03:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:53S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


### Changed By:

Last Name: HARTNETT

First Name: JAMES

MI: J

Signature: \_\_\_\_\_

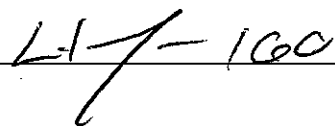

Badge No.: 160

Date: 02/11/2016

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02382	Calib. Date: 11/25/2015
Certification File No.:	02383	Calib. No.: 00029
Linearity File No.:	02384	Cert. Date: 11/25/2015
Solution File No.:	02412	Cert. No.: 00025
Sequential File No.:	02412	Lin. Date: 11/25/2015
		Lin. No.: 00024
		Soln. Date: 02/15/2016
		Soln. No.: 00242
		File Date: 02/15/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	14L135	Expires: 12/21/2016
		Bottle No.: 0072

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	00:18S		
Control 1 EC	0.099%	00:19S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	00:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:20S		
Control 2 EC	0.097%	00:20S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	00:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:21S		
Control 3 EC	0.097%	00:22S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	00:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	00:22S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: \_\_\_\_\_



Badge No.: 149

Date: 02/15/2016

# Calibrating Unit

## New Standard Solution Report

### Equipment

Alcotest 7110 MKIII-C  
Location: PENNSAUKEN TWSP. P.D.  
Serial No.: ARUM-0051  
Calibration File No.: 02382      Calib. Date: 11/25/2015      Calib. No.: 00029  
Certification File No.: 02383      Cert. Date: 11/25/2015      Cert. No.: 00025  
Linearity File No.: 02384      Lin. Date: 11/25/2015      Lin. No.: 00024  
Solution File No.: 02415      Soln. Date: 02/20/2016      Soln. No.: 00243  
Sequential File No.: 02415      File Date: 02/20/2016

Calibrating Unit: WET      Model No.: CU-34      Serial No.: DDUN S3-0338  
Control Solution %: 0.100%      Expires: 12/31/2016  
Solution Control Lot: 14L135      Bottle No.: 0074

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	08:08S		
Control 1 EC	0.099%	08:08S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	08:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:09S		
Control 2 EC	0.097%	08:10S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	08:10S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:10S		
Control 3 EC	0.097%	08:11S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	08:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:12S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: \_\_\_\_\_



Badge No.: 187

Date: 02/20/2016

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02418	Calib. Date: 03/01/2016
Certification File No.:	02419	Calib. No.: 00030
Linearity File No.:	02420	Cert. Date: 03/01/2016
Solution File No.:	02430	Cert. No.: 00026
Sequential File No.:	02430	Lin. Date: 03/01/2016
		Lin. No.: 00025
		Soln. Date: 03/17/2016
		Soln. No.: 00245
		File Date: 03/17/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	16A150	Expires: 01/05/2017
		Bottle No.: 1131

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	22:05S		
Control 1 EC	0.100%	22:06S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	22:06S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:07S		
Control 2 EC	0.098%	22:07S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	22:07S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:08S		
Control 3 EC	0.098%	22:09S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	22:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:09S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: SOTO

First Name: JESUS

MI: -

Signature: Pr J Soto 198

Badge No.: 198

Date: 03/17/2016

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02418	Calib. Date:	03/01/2016
Certification File No.:	02419	Cert. No.:	00030
Linearity File No.:	02420	Cert. Date:	03/01/2016
Solution File No.:	02438	Lin. Date:	03/01/2016
Sequential File No.:	02438	Lin. No.:	00025
		Soln. Date:	03/23/2016
		Soln. No.:	00246
		File Date:	03/23/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0338
Solution Control Lot:	16A150	Expires:	01/05/2017
		Bottle No.:	1269

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	23:16S		
Control 1 EC	0.101%	23:17S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	23:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:17S		
Control 2 EC	0.099%	23:18S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	23:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:19S		
Control 3 EC	0.098%	23:19S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	23:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:20S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: HENKEL

First Name: GERALD

MI: F.

Signature: \_\_\_\_\_

*Sgt M Henkel 149*

Badge No.: 149

Date: 03/23/2016

# Calibrating Unit

## New Standard Solution Report

**Equipment**

Alcotest 7110 MKIII-C		Serial No.: ARUM-0051
Location: PENNSAUKEN TWSP. P.D.		
Calibration File No.: 02418	Calib. Date: 03/01/2016	Calib. No.: 00030
Certification File No.: 02419	Cert. Date: 03/01/2016	Cert. No.: 00026
Linearity File No.: 02420	Lin. Date: 03/01/2016	Lin. No.: 00025
Solution File No.: 02442	Soln. Date: 03/26/2016	Soln. No.: 00247
Sequential File No.: 02442	File Date: 03/26/2016	
Calibrating Unit: WET	Model No.: CU-34	Serial No.: DDUN S3-0338
Control Solution %: 0.100%		Expires: 08/04/2017
Solution Control Lot: 15H140		Bottle No.: 1183

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	03:27S		
Control 1 EC	0.101%	03:28S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	03:28S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:29S		
Control 2 EC	0.099%	03:29S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	03:29S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:30S		
Control 3 EC	0.097%	03:31S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	03:31S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	03:32S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: HARTNETT

First Name: JAMES

MI: J

Signature: \_\_\_\_\_

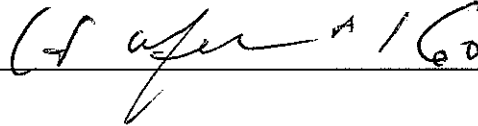

Badge No.: 160

Date: 03/26/2016

# Calibrating Unit

## New Standard Solution Report

### Equipment

Alcotest 7110 MKIII-C  
Location: PENNSAUKEN TWSP, P.D. Serial No.: ARUM-0051  
Calibration File No.: 02418 Calib. Date: 03/01/2016 Calib. No.: 00030  
Certification File No.: 02419 Cert. Date: 03/01/2016 Cert. No.: 00026  
Linearity File No.: 02420 Lin. Date: 03/01/2016 Lin. No.: 00025  
Solution File No.: 02444 Soln. Date: 03/26/2016 Soln. No.: 00248  
Sequential File No.: 02444 File Date: 03/26/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0338  
Control Solution %: 0.100% Expires: 01/05/2017  
Solution Control Lot: 16A150 Bottle No.: 1354

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	23:45S		
Control 1 EC	0.100%	23:46S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	23:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:47S		
Control 2 EC	0.099%	23:47S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	23:47S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:48S		
Control 3 EC	0.099%	23:49S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	23:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:50S		

All tests within acceptable tolerance.


On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: NURTHEN

First Name: RICHARD

MI: M

Signature:  #184

Badge No.: 184

Date: 03/26/2016



# Calibrating Unit

## New Standard Solution Report

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARUM-0051  
Location: PENNSAUKEN TWSP. P.D.  
Calibration File No.: 02418 Calib. Date: 03/01/2016 Calib. No.: 00030  
Certification File No.: 02419 Cert. Date: 03/01/2016 Cert. No.: 00026  
Linearity File No.: 02420 Lin. Date: 03/01/2016 Lin. No.: 00025  
Solution File No.: 02446 Soln. Date: 03/29/2016 Soln. No.: 00249  
Sequential File No.: 02446 File Date: 03/29/2016

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDUN S3-0338  
Control Solution %: 0.100% Expires: 08/04/2017  
Solution Control Lot: 15H140 Bottle No.: 1177

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	01:57S		
Control 1 EC	0.101%	01:57S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	01:57S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:58S		
Control 2 EC	0.098%	01:59S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	01:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:00S		
Control 3 EC	0.099%	02:00S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	02:00S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:01S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

### Changed By:

Last Name: FABIANI

First Name: P

MI: E

Signature: \_\_\_\_\_

*Handwritten signature: P F 187*

Badge No.: 187

Date: 03/29/2016

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP, P.D.	
Calibration File No.:	02418	Calib. Date: 03/01/2016
Certification File No.:	02419	Calib. No.: 00030
Linearity File No.:	02420	Cert. Date: 03/01/2016
Solution File No.:	02449	Cert. No.: 00026
Sequential File No.:	02449	Lin. Date: 03/01/2016
		Lin. No.: 00025
		Soln. Date: 04/01/2016
		Soln. No.: 00250
		File Date: 04/01/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0338
Solution Control Lot:	14F130	Expires: 06/20/2016
		Bottle No.: 0743

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	20:49S		
Control 1 EC	0.100%	20:49S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	20:49S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:50S		
Control 2 EC	0.098%	20:50S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	20:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:51S		
Control 3 EC	0.098%	20:52S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	20:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	20:53S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BRISTOW

First Name: MARK

MI: V

Signature: \_\_\_\_\_

*PTL. Bristow*

*#195*

Badge No.: 0195

Date: 04/01/2016

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02418	Calib. Date: 03/01/2016
Certification File No.:	02419	Calib. No.: 00030
Linearity File No.:	02420	Cert. Date: 03/01/2016
Solution File No.:	02470	Cert. No.: 00026
Sequential File No.:	02470	Lin. Date: 03/01/2016
		Lin. No.: 00025
		Soln. Date: 05/14/2016
		Soln. No.: 00252
		File Date: 05/14/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0339
Solution Control Lot:	201603L	Expires: 03/22/2018
		Bottle No.: 0180

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	06:55D		
Control 1 EC	0.102%	06:55D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.101%	06:55D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:56D		
Control 2 EC	0.100%	06:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	06:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:58D		
Control 3 EC	0.100%	06:58D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.102%	06:58D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:59D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BRISTOW

First Name: MARK

MI: V

Signature: \_\_\_\_\_

*PTL. Bristow #195*

Badge No.: 0195

Date: 05/14/2016

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02418	Calib. Date: 03/01/2016
Certification File No.:	02419	Calib. No.: 00030
Linearity File No.:	02420	Cert. Date: 03/01/2016
Solution File No.:	02494	Cert. No.: 00026
Sequential File No.:	02494	Lin. Date: 03/01/2016
		Lin. No.: 00025
		Soln. Date: 06/12/2016
		Soln. No.: 00253
		File Date: 06/12/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0339
Solution Control Lot:	201603L	Expires: 03/22/2018
		Bottle No.: 0881

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:30D		
Control 1 EC	0.103%	09:31D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	09:31D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:31D		
Control 2 EC	0.101%	09:32D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.103%	09:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:33D		
Control 3 EC	0.102%	09:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.104%	09:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:34D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: BRUNGES

First Name: MANDY

MI: L

Signature: \_\_\_\_\_

*[Handwritten Signature]* #176

Badge No.: 176

Date: 06/12/2016

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02418	Calib. Date: 03/01/2016
Certification File No.:	02419	Calib. No.: 00030
Linearity File No.:	02420	Cert. Date: 03/01/2016
Solution File No.:	02513	Cert. No.: 00026
Sequential File No.:	02513	Lin. Date: 03/01/2016
		Lin. No.: 00025
		Soln. Date: 07/14/2016
		Soln. No.: 00254
		File Date: 07/14/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0339
Solution Control Lot:	201605D	Expires: 05/17/2018
		Bottle No.: 0605

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:24D		
Control 1 EC	0.103%	13:24D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.102%	13:24D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:25D		
Control 2 EC	0.101%	13:26D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.102%	13:26D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:26D		
Control 3 EC	0.101%	13:27D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.102%	13:27D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:28D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: FABIANI

First Name: P

MI: E

Signature: \_\_\_\_\_

*P FABIANI 187*

Badge No.: 187

Date: 07/14/2016

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02418	Calib. Date: 03/01/2016
Certification File No.:	02419	Calib. No.: 00030
Linearity File No.:	02420	Cert. Date: 03/01/2016
Solution File No.:	02523	Cert. No.: 00026
Sequential File No.:	02523	Lin. Date: 03/01/2016
		Lin. No.: 00025
		Soln. Date: 08/21/2016
		Soln. No.: 00255
		File Date: 08/21/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0339
Solution Control Lot:	201605D	Expires: 05/17/2018
		Bottle No.: 0610

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	19:54D		
Control 1 EC	0.102%	19:55D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.102%	19:55D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:55D		
Control 2 EC	0.101%	19:56D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	19:56D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:57D		
Control 3 EC	0.101%	19:57D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	19:57D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:58D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: PASQUALE

First Name: JODY

MI:

Signature: \_\_\_\_\_



Badge No.: 199

Date: 08/21/2016

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02524	Calib. Date: 08/22/2016
Certification File No.:	02525	Calib. No.: 00031
Linearity File No.:	02526	Cert. Date: 08/22/2016
Solution File No.:	02543	Cert. No.: 00027
Sequential File No.:	02543	Lin. Date: 08/22/2016
		Lin. No.: 00026
		Soln. Date: 09/25/2016
		Soln. No.: 00257
		File Date: 09/25/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0339
Solution Control Lot:	201605D	Expires: 05/17/2018
		Bottle No.: 1201

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	06:13D		
Control 1 EC	0.104%	06:14D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.104%	06:14D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:15D		
Control 2 EC	0.103%	06:15D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.104%	06:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:16D		
Control 3 EC	0.103%	06:16D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.103%	06:16D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	06:17D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: KUCHMEK

First Name: JOSEPH

MI: -

Signature: \_\_\_\_\_



Badge No.: 216

Date: 09/25/2016

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02524	Calib. Date: 08/22/2016
Certification File No.:	02525	Calib. No.: 00031
Linearity File No.:	02526	Cert. Date: 08/22/2016
Solution File No.:	02556	Cert. No.: 00027
Sequential File No.:	02556	Lin. Date: 08/22/2016
		Lin. No.: 00026
		Soln. Date: 10/19/2016
		Soln. No.: 00258
		File Date: 10/19/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0339
Solution Control Lot:	201605D	Expires: 05/17/2018
		Bottle No.: 1202

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:12D		
Control 1 EC	0.104%	23:12D	34.0°C	CONTROL TEST FAILED
Control 1 IR	0.105%	23:12D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	23:13D		
Control 2 EC	0.103%	23:14D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.104%	23:14D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:15D		
Control 3 EC	0.103%	23:15D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.104%	23:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:16D		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: FABIANI

First Name: P

MI: E

Signature: \_\_\_\_\_



\*187

Badge No.: 187

Date: 10/19/2016



# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02524	Calib. Date: 08/22/2016
Certification File No.:	02525	Calib. No.: 00031
Linearity File No.:	02526	Cert. Date: 08/22/2016
Solution File No.:	02557	Cert. No.: 00027
Sequential File No.:	02557	Lin. Date: 08/22/2016
		Lin. No.: 00026
		Soln. Date: 10/20/2016
		Soln. No.: 00259
		File Date: 10/20/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0339
Solution Control Lot:	201605D	Expires: 05/17/2018
		Bottle No.: 1206

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	02:04D		
Control 1 EC	0.104%	02:05D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.104%	02:05D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:06D		
Control 2 EC	0.104%	02:06D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.104%	02:06D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:07D		
Control 3 EC	0.103%	02:08D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.104%	02:08D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	02:08D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: FABIANI

First Name: P

MI: E

Signature: \_\_\_\_\_



Badge No.: 187

Date: 10/20/2016

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02524	Calib. Date:	08/22/2016
Certification File No.:	02525	Cert. No.:	00031
Linearity File No.:	02526	Cert. Date:	08/22/2016
Solution File No.:	02563	Lin. No.:	00026
Sequential File No.:	02563	Soln. Date:	10/30/2016
		Soln. No.:	00260
		File Date:	10/30/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0339
Solution Control Lot:	16140	Expires:	06/07/2018
		Bottle No.:	1443

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	01:57D		
Control 1 EC	0.102%	01:58D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.103%	01:58D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:59D		
Control 2 EC	0.101%	01:59D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	01:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:00S		
Control 3 EC	0.101%	01:01S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	01:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	01:01S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: FABIANI

First Name: P

MI: E

Signature: \_\_\_\_\_

*[Handwritten Signature]* #187

Badge No.: 187

Date: 10/30/2016

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02524	Calib. Date: 08/22/2016
Certification File No.:	02525	Calib. No.: 00031
Linearity File No.:	02526	Cert. Date: 08/22/2016
Solution File No.:	02572	Cert. No.: 00027
Sequential File No.:	02572	Lin. Date: 08/22/2016
		Lin. No.: 00026
		Soln. Date: 12/02/2016
		Soln. No.: 00261
		File Date: 12/02/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0339
Solution Control Lot:	15H140	Expires: 08/04/2017
		Bottle No.: 1179

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	19:10S		
Control 1 EC	0.106%	19:11S	34.0°C	CONTROL TEST FAILED
Control 1 IR	0.102%	19:11S	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	19:11S		
Control 2 EC	0.104%	19:12S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	19:12S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:13S		
Control 3 EC	0.103%	19:13S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	19:13S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	19:14S		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: KUCHMEK

First Name: JOSEPH

MI: -

Signature: \_\_\_\_\_



Badge No.: 216

Date: 12/02/2016

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.		
Calibration File No.:	02524	Calib. Date:	08/22/2016
Certification File No.:	02525	Cert. No.:	00031
Linearity File No.:	02526	Cert. Date:	08/22/2016
Solution File No.:	02573	Lin. No.:	00027
Sequential File No.:	02573	Lin. Date:	08/22/2016
		Soln. No.:	00026
		Soln. Date:	12/05/2016
		File Date:	12/05/2016
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDUN S3-0339
Solution Control Lot:	15H140	Expires:	08/04/2017
		Bottle No.:	1181

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:54S		
Control 1 EC	0.105%	23:55S	34.0°C	CONTROL TEST FAILED
Control 1 IR	0.102%	23:55S	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	23:56S		
Control 2 EC	0.103%	23:56S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	23:56S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:57S		
Control 3 EC	0.103%	23:58S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.102%	23:58S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:58S		

Test results are not within acceptable range.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

**Changed By:**

Last Name: FABIANI

First Name: P

MI: E

Signature: \_\_\_\_\_



Badge No.: 187

Date: 12/05/2016

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARUM-0051
Location:	PENNSAUKEN TWSP. P.D.	
Calibration File No.:	02524	Calib. Date: 08/22/2016
Certification File No.:	02525	Calib. No.: 00031
Linearity File No.:	02526	Cert. Date: 08/22/2016
Solution File No.:	02574	Cert. No.: 00027
Sequential File No.:	02574	Lin. Date: 08/22/2016
		Lin. No.: 00026
		Soln. Date: 12/07/2016
		Soln. No.: 00263
		File Date: 12/07/2016
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDUN S3-0339
Solution Control Lot:	15H140	Expires: 08/04/2017
		Bottle No.: 1181

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:07S		
Control 1 EC	0.103%	16:08S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	16:08S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:09S		
Control 2 EC	0.101%	16:09S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	16:09S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:10S		
Control 3 EC	0.100%	16:11S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	16:11S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	16:11S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: SULZBACH

First Name: CHRIS

MI: L

Signature: \_\_\_\_\_

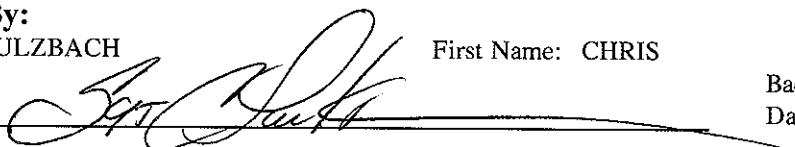

Badge No.: 127

Date: 12/07/2016